

November 2012

# Efficacy of miniaturized imacor trans-esophageal echocardiogram (TEE) prove in mechanical circulatory support.

Hitoshi Hirose

*Thomas Jefferson University, Hitoshi.Hirose@jefferson.edu*

Christopher Y. Kang

*Thomas Jefferson University, christopher.kang@jefferson.edu*

Joshua K. Wong

*Thomas Jefferson University*

Harrison T. Pitcher

*Thomas Jefferson University, Harrison.pitcher@jefferson.edu*

Caitlyn M. Johnson

*Thomas Jefferson University, Caitlyn.Johnson@jefferson.edu**See next page for additional authors*

## [Let us know how access to this document benefits you](#)

Follow this and additional works at: <http://jdc.jefferson.edu/surgeryfp>Part of the [Surgery Commons](#)

### Recommended Citation

Kang CY, Johnson CM, Pitcher H, Hirose H, Cavarocchi NC. Efficacy of miniaturized imacor trans-esophageal echocardiogram (TEE) prove in mechanical circulatory support. Presented at the 58th Annual Conference American Society of Artificial Organs. San Francisco, CA. June 13-16, 2012.

This Article is brought to you for free and open access by the Jefferson Digital Commons. The Jefferson Digital Commons is a service of Thomas Jefferson University's [Center for Teaching and Learning \(CTL\)](#). The Commons is a showcase for Jefferson books and journals, peer-reviewed scholarly publications, unique historical collections from the University archives, and teaching tools. The Jefferson Digital Commons allows researchers and interested readers anywhere in the world to learn about and keep up to date with Jefferson scholarship. This article has been accepted for inclusion in Department of Surgery Faculty Papers by an authorized administrator of the Jefferson Digital Commons. For more information, please contact: [JeffersonDigitalCommons@jefferson.edu](mailto:JeffersonDigitalCommons@jefferson.edu).

---

**Authors**

Hitoshi Hirose, Christopher Y. Kang, Joshua K. Wong, Harrison T. Pitcher, Caitlyn M. Johnson, Konrad Sarosiek, Linda J Bogar, and Nicholas C. Cavarocchi

# Application of the Miniaturized ImaCor Trans-Esophageal (TEE) Probe in Heart Transplant/Mechanical Cardiac Support Patients

Christopher Y. Kang, MD, Joshua K. Wong, BS, Harrison T. Pitcher, MD, Caitlyn Johnson, MD, Konrad Sarosiek, MD, Linda Bogar, MD, Hitoshi Hirose, MD, Nicholas C. Cavarocchi, MD

Department of Surgery, Division of Cardiothoracic Surgery, Thomas Jefferson University Hospital, Philadelphia, PA, United States

## Introduction

In the surgical cardiac intensive care unit (ICU), therapeutic interventions often need to be done at the bedside, necessitating the need for a rapidly employable diagnostic tool for the cardiac intensivist. Cardiac function and volume status are critical components to patient care. Intravascular volume status is difficult to establish. Current modalities use indirect methods to gather data which can misdirect patient care. Conventional TTE and TEE are unsuitable for continuous and effective hemodynamic assessment.

## ImaCor hTEE Probe

- A miniaturized TEE probe
- FDA approved
- Real time monitoring, able to use for 72 hours continuously.
- Allows direct visualization of intravascular volume and cardiac function
- No need of anesthesia or sedation.

## Methods

IRB approved retrospective review of mechanical circulatory support patients and post heart transplant patients who had ImaCor TEE (hTEE) monitoring in ICU.

3 categories of intervention based on hTEE

**Major:** Tamponade, ECMO wean

**Moderate:** Device wean, inotrope management, fluid and hemodynamic management

**Minor:** ECMO cannula placement, other data

## Contact

Nicholas C. Cavarocchi, MD  
Associate Professor Of Surgery  
Critical Care Director, Surgical Intensive Care Unit  
nicholas.cavarocchi@jefferson.edu

## Results

N = 34 patients with hTEE monitoring

N = 21 post MCS or HTX

- Age: 28-73, Median : 49, Sex: M: 14 F: 7
- Devices employed:6
  - ECMO: 13
  - Post LVAD: 9
  - Impella: 3
  - Post HTX: 4
  - Pts with multiple: 6



		Pre-hTEE Dx	Post-hTEE Dx	Intervention	
<b>Major (n=4, 19%)</b>	Post Heart TX	Hemodynamic Instability (n=1)	Tamponade (n=1)	Operative Evacuation	
	MCS (ECMO/VAD)	ECMO Wean (n=3)	Biventricular failure (n=3)	Contraindication of LVAD, Withdraw of Care	
<b>Moderate (n=13, 62%)</b>	Post Heart TX	Hemodynamic Instability (n=6)	RV Failure (n=4)	Increased Fluids, Inotrope management	
			No Tamponade (n=2)	Medical management	
	MCS (ECMO/VAD)	Hemodynamic Instability (n= 4)	ECMO Wean (n=3)	Recoverable RV function (n=3)	LVAD
			Myocardial Hematoma without perforation (n=1)	Observation	
<b>Minor (n=4, 19%)</b>	MCS (ECMO/VAD)	Hemodynamic Instability (n=4)	Inadequate VAD flow (n=1)	Increased VAD speed	
			RV Failure post VAD (n=2)	Inotrope management	
			No LV thrombus (n=1)	Observation	
			ECMO venous cannula Clot (n=1)	Reposition	
			ECMO cannula malposition (n=2)	Emergent Bedside Reposition	

## Financial

The cost difference between this new device and the traditional TEE is also significant (\$900 USD vs \$4600 USD). Our institution saved in excess of \$150,000 USD with the use of this device instead of traditional TEE.

### ImaCor hTEE


- Device : \$65,000
- Probe : \$900

**TTE** : Prof fee \$185, Technical fee \$2332

**TEE** : Prof fee \$380, Technical fee \$3906

Not including technician basic after hour call in charge of \$225 per echo.

### Comparative Cost of Conventional TEE vs. hTEE for 5 studies in 72 hours

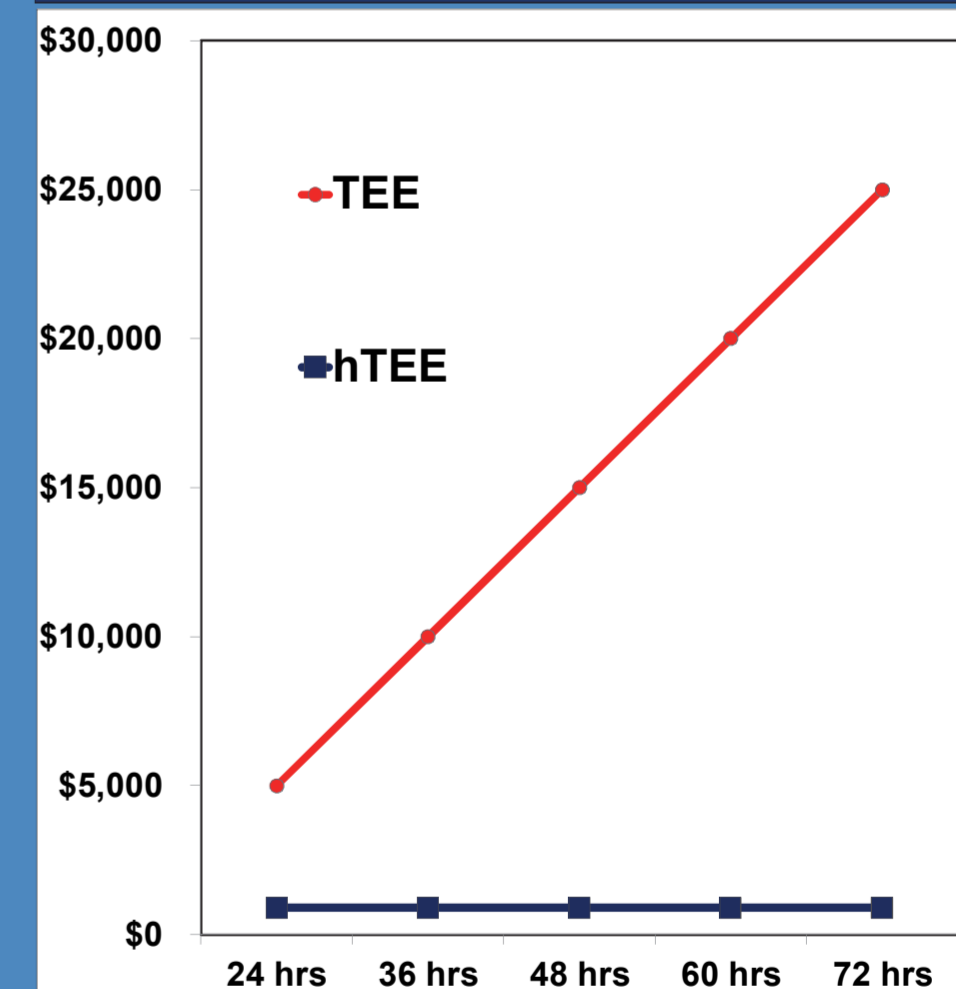

## Conclusions

This device has proven to be an invaluable new adjunct in the ICU by allowing previously unobtainable continuous real time monitoring of MCS/Post HTX.

The use of the ImaCor hTEE probe provides the intensivist with timely important clinical data that improves patient care and is economically advantageous. Using serial hTEE data, the clinician can reliably make accurate decisions in regards to operative interventions.